



 swiss hand made

LABORATORY ELECTRODES

- ▶ *pH Electrodes*
- ▶ *Conductivity Cells*
- ▶ *Calibration Buffers*

▶ Electrode selection table

	GEL	POLYMER	POLYMER TIP	STANDARD	20IT / POLYMER PLAST	STANDARD HA	FLAT	STANDARD HF	FOOD	2 PORE SLIM	2 PORE	2 PORE F	FOOD SLIM	SEMIMICRO	MICRO	MICRO P	MICRO SPECIAL	FLOW
Waste water		●	●		●	●												●
Deionized water									●									●
Tap water	●	●	●	●	●				●									●
Food									●	●	●	●	●					
Butter									●	●	●	●	●					
Samples with protein		●	●						●		●		●			●		
Alkali samples						●												
High temperature samples				●		●			●									
Samples in tube for NMR																	●	
small volume samples							●								●	●	●	
Samples with Hydrofluoric acid								●										
Viscous samples		●	●						●									●
Cosmetics		●	●	●		●			●									●
Cream		●	●						●									●
Detergents	●	●	●	●	●	●			●									●
Aqueous emulsions		●	●	●					●									●
Cheese										●	●	●	●					
Fruit and vegetables										●	●	●	●					
Milk		●	●						●	●	●	●	●					
Mayonnaise									●		●							●
Marmalade		●	●						●		●							●
Bread and pasta			●						●	●	●	●	●					
Leather							●											
Brine	●	●	●	●	●				●									●
Soap		●	●	●					●									●
Samples with low ionic strenght																		●
Aqueous suspensions		●	●	●					●									●
Semi Aqueous suspensions									●									●
Fruit juice		●	●	●					●									●
Surfaces							●											
TRIS swab				●														●
Tip			●							●	●	●	●					●
Titolation				●					●									●
Non Aqueous titolation																		●
Galvanic treatment		●	●			●												●
Water-based paints		●	●	●					●									●
Paints				●					●									●
Wine		●	●	●					●									●
Yogurt		●	●						●	●	●	●	●					●

► Quality test certificate

XS electrodes Standard and Flow are provided with a quality certificate attesting and documents the final inspection, carried out on each single electrode. On the certificate and on the label is stated the serial number of the electrode for a correct traceability (GLP) of the calibrations and of the measurement chain.


Electrode model

Production batch

Tests results

Technical specifications

Test date

 QUALITY TEST REPORT	
Electrode Type: <i>Elektrodentyp / Elettrodo</i>	STANDARD
Product number: <i>Produktnummer / Codice prodotto</i>	32200373
Serial number: <i>Seriennummer / Numero seriale</i>	0009
Batch number: <i>Chargennummer / Numero di lotto</i>	444
Reading in pH 7 buffer ($0 \pm 20\text{mV}$): <i>Lesen im pH 7 / Lettura in pH 7*</i>	-5 mV
Reading in pH 4 buffer ($174 \pm 20\text{mV}$): <i>Lesen im pH 4* / Lettura in pH 4*</i>	169 mV
Measuring range: <i>Messbereich / Range di misura</i>	0...14 pH
Temperature range: <i>Temperaturbereich / Range di temperatura</i>	-10...80 °C
Temperature sensor: <i>Temperatursensor / Sensore di temperatura</i>	
Reference electrolyte: <i>Bezugselektrolyt / Elettrolita di riferimento</i>	KCl 3M
<small>* Measurements are performed in Certified Reference Materials. * Die Messungen werden in zertifizierten Referenzmaterialien durchgeführt. * Le misurazioni sono eseguite in materiali di riferimento certificati</small>	
<small>A change of the measurement values above during storage and use is a normal behavior of the electrochemical sensors. Eine Änderung der Meßwerte oberhalb während der Lagerung und der Verwendung ist ein normales Verhalten der elektrochemischen Sensoren. Una variazione dei valori di misura di cui sopra, durante la conservazione e l'uso, è un comportamento normale dei sensori elettrochimici.</small>	
Passed Quality Control <i>Bestanden Qualitätskontrolle / Controllo Qualità Effettuato</i>	16/02/2018
<small>This document is generated electronically and doesn't require any signature. Dieses Dokument ist elektronisch erzeugt und erfordert keine Unterschrift erforderlich. Questo documento è generato elettronicamente e non richiede alcuna firma.</small>	



Electrode box with instruction printed on box



Indelible internal serial number

▶ XS Sensor electrodes

Very famous Swiss producer has developed a complete line of laboratory pH, Redox and conductivity electrodes, with glass and plastic body. The new XS sensor are available with S7 head or fix cable with BNC or DIN connector plug. For food application many models are equipped with temperature sensor inside, for fast temperature compensation. Some models are designed to help in daily work in GLP condition with indelible internal serial number and quality certificate.



Serial number



Violet inner buffer

Special polymer electrolyte, combined with high performance reference system, generate a complete range of electrodes for food application, in special part of this catalogue.

Blue inner buffer provides clear visual of contact with internal pH glass membrane.

All XS sensors are connectable to all common pHmeters in the market. Our customer support is available for every special application request, or support for the selection of the right electrode.

XS sensor are the perfect solutions for pH measurements, if combined with XS pH meters and XS buffer solutions.

DHS Digital High Sensor Intelligent sensors management

Digital High Sensors are the new pH sensors with internal chip, that store parameters, date of last calibration, model and production batch of the electrode. In the instruments with DHS function is inserted a special chip with the same technology. After connecting the pH DHS sensor to the instrument, all the data stored in the sensor chip are automatically transferred to the instrument. The display will show in a screen: DHS, sensor model, production batch, date and hour of the last calibration.



MEAS pH		25/10/2018 15:57:01
Connected DHS pH Sensor		
DHS Sensor	Std	
Batch	738	
Calibration date	19/10/2017	
Calibration Hour	09:02	

After a new calibration of the DHS electrode, the data is automatically stored in the electrode chip. If we move this electrode to another DHS-enabled instrument, we can start working immediately and with extreme security as the data from the last calibration will automatically be transferred and used for pH measurements.

New DHS pH sensors do not have an internal battery so they can be stored as a normal pH electrode and do not use special connectors but a normal BNC.

Many manufacturers using digital sensors have developed dedicated meters for these sensors. This imposes a full range of digital sensors for a variety of applications or lab requirements. Our research and development team has designed this new line of instruments to work with the new DHS digital sensors and the normal analog pH sensors both, all brands, which can be connected to the same pH meter.

From now on, the pH measurement will be simpler.


Cables



1 m cable S7 / BNC - Code **33551733**



1 m cable S7 / DIN - Code **33551743**

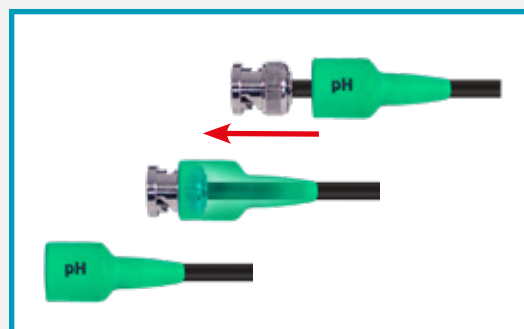

BNC plug with plastic protection

► DHS DIGITAL ELECTRODES



Model	201 T DHS	Standard T-BNC DHS	Flow Temp DHS	2 Pore T DHS	2 Pore F Temp DHS
	For portable meter	For bench meter		Food measurement application	
Code	32200103	32200123	32200133	32200113	32200143
Head	Cable fix / BNC	Cable fix / BNC	Cable fix / BNC	Cable fix / BNC	Cable fix / BNC
pH range	0...14	0...14	0...14	0...14	0...14
Temperature range	0...60 °C	-10...100 °C	-10...80 °C	0...60 °C	0...60 °C
Temperature sensor	Yes/plug RCA Cinch	Yes/plug RCA Cinch	Yes/plug RCA Cinch	Yes/plug RCA Cinch	Yes/plug RCA Cinch
Shaft material	Epoxy	Glass	Glass	Glass	POM/Glass
Diaphragm	Ceramic	Ceramic	Teflon sleeve	2 open pore	2 open pore
Reference system	Ag/AgCl	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag coated	Ag coated
Electrolyte	Gel	KCl 3M	KCl 3M	Polymer	Polymer
Shaft length	120 mm	120 mm	120 mm	95 mm / 35 mm	90 mm / 50 mm
Shaft diameter	12 mm	12 mm	12 mm	12 mm / 6 mm	12 mm / 6 mm
Note / Application	Temperature sensor NTC 30 K Ω . Maintenance free	Temperature sensor NTC 30 K Ω . With serial number and certificate. General application	Temperature sensor NTC 30 K Ω . With serial number and certificate. Viscous sample and low ion media	Temperature sensor NTC 30 K Ω . For food application, meat and cheese	Temperature sensor NTC 30 K Ω . For food application, meat and cheese with epoxy body

▶ GENERAL LABORATORY APPLICATION







+ swiss hand made

Model	Polymer	Polymer TIP	Gel	Standard BNC	Standard DIN
Code	32200223	32200443	32200203	32200263	32200273
Head	S7 connector	S7 connector	S7 connector	Cable fix / BNC	Cable fix / DIN
pH range	0...14	0...14	0...14	0...14	0...14
Temperature range	-10...80 °C	-10...80 °C	-10...60 °C	-10...100 °C	-10...100 °C
Temperature sensor	No	No	No	No	No
Shaft material	Glass	Glass	Glass	Glass	Glass
Diaphragm	Open pore	2 open pore	Ceramic	Ceramic	Ceramic
Reference system	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl	Ag/AgCl Cartridge	Ag/AgCl Cartridge
Electrolyte	Polymer	Polymer	Gel	KCl 3M	KCl 3M
Shaft length	120 mm	120 mm	120 mm	120 mm	120 mm
Shaft diameter	12 mm	12 mm	12 mm	12 mm	12 mm
Note / Application	Maintenance free	For pH soil measurement	Maintenance free	With serial number and certificate. General application	With serial number and certificate. General application

▶ GENERAL LABORATORY APPLICATION



+ swiss hand made

					
Model	Standard T-BNC	Standard T-DIN	Standard	Standard HA	Standard HF
Code	32200473	32200463	32200363	32200423	32200433
Head	Cable fix / BNC	Cable fix / DIN	S7 connector	S7 connector	S7 connector
pH range	0...14	0...14	0...14	0...14	0...14
Temperature range	-10...100 °C	-10...100 °C	-10...100 °C	-10...100 °C	-10...100 °C
Temperature sensor	Yes/plug RCA Cinch	Yes/spina Banana 4 mm	No	No	No
Shaft material	Glass	Glass	Glass	Glass	Glass
Diaphragm	Ceramic	Ceramic	Ceramic	Ceramic	Ceramic
Reference system	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl Cartridge
Electrolyte	KCl 3M	KCl 3M	KCl 3M	KCl 3M	KCl 3M
Shaft length	120 mm	120 mm	120 mm	120 mm	120 mm
Shaft diameter	12 mm	12 mm	12 mm	12 mm	12 mm
Note / Application	Temperature sensor NTC 30 KΩ	Temperature sensor NTC 30 KΩ	With serial number and certificate. General application	With serial number and certificate. Minimal alkali error	For sample with HF (0,01 M / 200 mg/l)

▶ GENERAL LABORATORY APPLICATION

swiss hand made



				
Model	Flat	Flow	Flow Temp BNC	Flow Temp DIN
Code	32200413	32200373	32200723	32200733
Head	S7 connector	S7 connector	Cable fix / BNC	Cable fix / DIN
pH range	0...14	0...14	0...14	0...14
Temperature range	0...60 °C	-10...80 °C	-10...80 °C	-10...80 °C
Temperature sensor	No	No	Yes/plug RCA Cinch	Yes/Banana 4 mm plug
Shaft material	Glass	Glass	Glass	Glass
Diaphragm	Teflon with 3 open pore	Teflon sleeve	Teflon sleeve	Teflon sleeve
Reference system	Ag coated	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl Cartridge
Electrolyte	Polymer	KCl 3M	KCl 3M	KCl 3M
Shaft length	120 mm	120 mm	120 mm	120 mm
Shaft diameter	12 mm	12 mm	12 mm	12 mm
Note / Application	For surface measurement e. g. paper and skin	With serial number and certificate. Viscous sample and low ion media	Temperature sensor NTC 30 KΩ. With serial number and certificate. Viscous sample and low ion media	Temperature sensor PT 1000. With serial number and certificate. Viscous sample and low ion media

▶ GENERAL LABORATORY APPLICATION



swiss hand made

Model	Semi Micro	Micro	Micro P	Micro Special
Code	32200383	32200213	32200253	32200453
Head	S7 connector	S7 connector	S7 connector	S7 connector
pH range	0...14	0...14	0...14	0...14
Temperature range	0...100 °C	0...100 °C	0...100 °C	0...100 °C
Temperature sensor	No	No	No	No
Shaft material	Glass	Glass	Glass	Glass
Diaphragm	Ceramic	Ceramic	Ceramic	Ceramic
Reference system	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl Cartridge
Electrolyte	KCl 3M	KCl 3M	Glicerina KCl	KCl 3M
Shaft length	150 mm / 100 mm	120 mm / 60 mm	120 mm / 60 mm	220 mm / 180 mm
Shaft diameter	12 mm / 6 mm	12 mm / 3 mm	12 mm / 3 mm	12 mm / 3 mm
tubeNote / Application	Test tube measurement	Small volume sample < 2 ml	Small volume sample < 2 ml with protein	Measure in NMR tube

▶ FOOD MEASUREMENT APPLICATION



swiss hand made

Model	Zetatrode	Food	Food Slim	2 Pore Steel	2 Pore Steel T	2 Pore Steel T DIN	2 Pore K complete	2 Pore K without knife
Code	32200403	32200393	32200243	32200653	32200313	32200643	32200303	32200343
Head	S7 connector	S7 connector	S7 connector	S7	Cable fix / BNC	Cable fix / DIN	S7 connector	S7 connector
pH range	0...14	0...14	0...14	0...14			0...14	0...14
Temperature range	0...60 °C	-10...100 °C	0...100 °C	0...80 °C			0...60 °C	0...60 °C
Temperature sensor	No	No	No		Yes/plug RCA Cinch	Yes/Banana 4 mm plug	No	No
Shaft material	Glass	Glass	Glass	Glass/ Polish steel			Glass/ Polish steel	Glass/ Polish steel
Diaphragm	Ceramic	3 ceramici	2 ceramici	2 open pore			2 open pore	2 open pore
Reference system	Ag/AgCl	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag coated			Ag coated	Ag coated
Electrolyte	Glicerina KCl	Glicerina KCl	Glicerina KCl	Polymer			Polymer	Polymer
Shaft length	190 mm / 120 mm	120 mm	95 mm / 25 mm	105 mm / 50 mm			110 mm / 35 mm	110 mm / 35 mm
Shaft diameter	12 mm / 4 mm	12 mm	12 mm / 6 mm	12 mm / 6 mm			12 mm / 4,5 mm	12 mm / 4,5 mm
Note / Application	For cheese measure	For food and cheese application	Fore spear measure	Penetration tip for hard samples			With knife	without knife. Replaceable knife Code: 32200353

▶ FOOD MEASUREMENT APPLICATION



swiss hand made

Model	2 Pore	2 Pore Slim	2 Pore F	2 Pore F Temp BNC	2 Pore F Temp DIN	2 Pore T
Code	32200333	32200283	32200293	32200703	32200713	32200323
Head	S7 connector	S7 connector	S7 connector	Cable fix/BNC	Cable fix/DIN	Cable fix/BNC
pH range	0...14	0...14	0...14	0...14	0...14	0...14
Temperature range	0...60 °C	0...60 °C	0...60 °C	0...60 °C	0...60 °C	0...60 °C
Temperature sensor	No	No	No	Yes/plug RCA Cinch	Yes/Banana 4 mm plug	Yes/plug RCA Cinch
Shaft material	Glass	Glass	POM/Glass	POM/Glass	POM/Glass	Glass
Diaphragm	2 open pore	2 open pore	2 open pore	2 open pore	2 open pore	2 open pore
Reference system	Ag coated	Ag coated	Ag coated	Ag coated	Ag coated	Ag coated
Electrolyte	Polymer	Polymer	Polymer	Polymer	Polymer	Polymer
Shaft length	100 mm / 35 mm	100 mm / 35 mm	90 mm / 50 mm	90 mm / 50 mm	90 mm / 50 mm	95 mm / 35 mm
Shaft diameter	12 mm / 6 mm	12 mm / 4,5 mm	12 mm / 6 mm	12 mm / 6 mm	12 mm / 6 mm	12 mm / 6 mm
Note / Application	For meat and cheese spear application	For meat and cheese spear application	For meat and cheese spear application	Temperature sensor NTC 30 KΩ	Temperature sensor PT 1000	Temperature sensor NTC 30 KΩ

▶ pH PLASTIC SHAFT ELECTRODES

+ swiss hand made



Model	Polymer Plast	Polymer Plast BNC	Polymer Plast DIN	 201 T	 201 T DIN
Code	32200493	32200503	32200513	50002002	50002052 50002042
Head	S7 connector	Cable fix/BNC	Cable fix/DIN	Cable fix/BNC	Cable fix/DIN
pH range	0...14	0...14	0...14	0...14	0...14
Temperature range	0...60 °C	0...60 °C	0...60 °C	0...60 °C	0...60 °C
Temperature sensor	No	No	No	Yes/plug RCA Cinch	1 banana 4 mm 2 banana 4 mm
Shaft material	Epoxy	Epoxy	Epoxy	Epoxy	Epoxy
Diaphragm	1 Ceramic + 1 open pore	1 Ceramic + 1 open pore	1 Ceramic + 1 open pore	Ceramic	Ceramic
Reference system	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl Cartridge	Ag/AgCl	Ag/AgCl
Electrolyte	Polymer	Polymer	Polymer	Gel	Gel
Shaft length	120 mm	120 mm	120 mm	120 mm	120 mm
Shaft diameter	12 mm	12 mm	12 mm	12 mm	12 mm
Note / Application	Maintenance free	Maintenance free	Maintenance free	Temperature sensor NTC 30 KΩ	Temperature sensor NTC 30 KΩ

▶ ORP ELECTRODES



+ swiss hand made

Model	Plast ORP	Plast ORP BNC	Standard Ag	Standard ORP	Standard KF
Code	32200663	32200673	32200483	32200233	32200523
Head	S7 connector	Cable fix/BNC	S7 connector	S7 connector	S7 connector
mV range	±1000	±1000	±2000	±2000	-
Temperature range	0...60 °C	0...60 °C	-10...80 °C	-10...100 °C	0...80 °C
Temperature sensor	No	No	No	No	No
Shaft material	Epoxy	Epoxy	Glass	Glass	Glass
Diaphragm	Ceramic	Ceramic	Ceramic	3 ceramics	-
Reference system	Ag/AgCl double junction	Ag/AgCl double junction	Ag/AgCl Cartridge	Ag/AgCl Cartridge	-
Electrolyte	Gel	Gel	KNO ₃ 1M	KCl 3M	-
Shaft length	120 mm	120 mm	120 mm	120 mm	120 mm
Shaft diameter	12 mm	12 mm	12 mm	12 mm	12 mm
Note / Application	Platinum pin for REDOX measurement	Platinum pin for REDOX measurement	Silver pin for argentometric titration	Platinum ring for REDOX measurement	Double platinum pin for KF e SO ₂ titration

▶ CONDUCTIVITY CELLS



	🌡️		🌡️		🌡️	
Model	VP 1	VPT 1	VPT 01	VPT 10	VPT 10 H	2301 T
Code	50004062	50003352	50004012	50004072	50003372	50004002
Head	Cable fix/BNC		Cable fix/BNC		Cable fix/BNC	
COND range	10 µS...10 mS		0,1 µS...1 mS		100 µS...500 mS	
Temperature range	0...80 °C		0...60 °C		0...80 °C	
Temperature sensor	No	Yes/plug RCA Cinch	Yes/plug RCA Cinch	Yes/plug RCA Cinch	Yes/plug RCA Cinch	Yes/plug RCA Cinch
Shaft material	Glass		PVC/Polish steel		Glass	
Plate	Platinum		Steel		Platinum	
Shaft length	120 mm		120 mm		120 mm	
Shaft diameter	12 mm		12 mm		12 mm	
Note / Application	Cell constant C=1 Temperature sensor NTC 30 KΩ (VPT 1)		Cell constant C=0,1 Temperature sensor NTC 30 KΩ. For ultrapure water		Cell constant C=10 Temperature sensor NTC 30 KΩ. For sea water	
					For high conductivity	

ELECTROLYTE AND MAINTENANCE SOLUTIONS

Code	Package	Description
32208113	75 ml	Solution KCl 3M + AgCl
12005033	100 ml	Solution 1M LiCl in Etilic alcool
32208003	75 ml	Solution 3M KCl
32208013	500 ml	Solution 3M KCl
32208023	75 ml	Solution GLYCERIN-KCl
32208033	75 ml	Solution KNO ₃ 1M for electrode STANDARD Ag
32208043	75 ml	Solution STORAGE for electrodes
32208053	500 ml	Solution STORAGE for electrodes
32208063	75 ml	Cleaning solution PROTEIN (pepsina) for electrodes Food application
32208093	250 ml	Cleaning solution PROTEIN (pepsina) for electrodes Food application
32208073	75 ml	Cleaning solution DIAPHRAGM (thiourea)
32208103	250 ml	Cleaning solution DIAPHRAGM (thiourea)
32208083	75 ml	RIGENERATION solution (with HF) for pH electrodes

swiss hand made

► CALIBRATION BUFFERS pH - Conductivity - Redox



Buffer solutions

- 250 ml and 500 ml ergonomic bottle with built-in dosing compartment and value table depending on temperature for an accurate calibration
- Economical, using just the proper amount per calibration
- Coloured for an easier identification
- Immune to micro-organisms
- Life time 36 months
- Actual value and expiration date printed on the bottle
- Actual value and expiration date reported on the certificate
- Certificates available at our website

XS Professional with DAKKS/DKD certificate

pH BUFFERS				
Code	Package	pH value (25°C)	Accuracy	Color
51300003	250 ml	4,01	± 0,01	Red
51300013	250 ml	7,00	± 0,01	Green
51300023	250 ml	9,21	± 0,02	Blue
51300033	250 ml	10,01	± 0,02	Yellow
51300103	500 ml	4,01	± 0,01	Red
51300113	500 ml	7,00	± 0,01	Green
51300123	500 ml	9,21	± 0,02	Blue
51300133	500 ml	10,01	± 0,02	Yellow

XS Basic with NIST certificate referred

pH BUFFERS				
Code	Package	pH value (25°C)	Accuracy	Color
51100033	250 ml	4,01	± 0,01	Red
51100043	250 ml	7,00	± 0,01	Green
51100053	250 ml	9,00	± 0,02	Blue
51100073	250 ml	9,21	± 0,02	Blue
51100063	250 ml	10,01	± 0,02	colourless
51100133	500 ml	4,01	± 0,01	Red
51100143	500 ml	7,00	± 0,01	Green
51100153	500 ml	9,00	± 0,02	Blue
51100173	500 ml	9,21	± 0,02	Blue
51100163	500 ml	10,01	± 0,02	colourless
51100233	5 l	4,01	± 0,01	Red
51100243	5 l	7,00	± 0,01	Green
51100253	5 l	9,00	± 0,02	Blue
51100273	5 l	9,21	± 0,02	Blue
51100263	5 l	10,01	± 0,02	colourless

pH and conductivity sachet buffer solutions 25 ml with NIST certificate



Conductivity Standards

- 500 ml ergonomic bottle with built-in dosing compartment and value table depending on temperature for an accurate calibration
- 1,3 and 5,0 µS/cm in 300 ml glass bottle
- Economical, using just the proper amount per calibration
- Life time 24 months
- 1,3 and 5,0 µS/cm life time minimum 12 months
- Actual value and expiration date printed on the bottle
- Actual Value and expiration date reported on the certificate
- Certificates available at our website

XS Professional with DANAK/DFM certificate

CONDUCTIVITY STANDARD			
Code	Package	value µS/cm (20°C / 25°C)	Accuracy
51300303	300 ml	1,3	± 0.1 µS/cm
51300313	300 ml	5,0	± 0.1 µS/cm
51300323	500 ml	76 / 84	± 1%
51300333	500 ml	133 / 147	± 1%
51300343	500 ml	1278 / 1413	± 1%
51300353	500 ml	11670 / 12880	± 1%

XS Basic with NIST certificate referred

CONDUCTIVITY STANDARD			
Code	Package	value µS/cm (20°C / 25°C)	Accuracy
51100503	300 ml	1,3	± 0.1 µS/cm
51100513	300 ml	5,0	± 0.1 µS/cm
51100613	500 ml	76 / 84	± 1%
51100623	500 ml	133 / 147	± 1%
51100633	500 ml	1278 / 1413	± 1%
51100643	500 ml	11670 / 12880	± 1%



Fill calibration compartment with simple press



Calibrate electrode



Empty calibration compartment

REDOX STANDARD For check ORP electrode

Code	Package	mV Value	Accuracy
51100303	250 ml	Redox/ORP 200mV/25°C	± 5mV
51100313	250 ml	Redox/ORP 475mV/25°C	± 5mV
51100323	500 ml	Redox/ORP 475mV/25°C	± 5mV
51100333	5 l	Redox/ORP 650mV/25°C	± 5mV

► Start with right solution

XS
INSTRUMENTS



Giorgio Bormac Company specialist in electrochemistry has developed this new line of instruments, finding the right balance between the design, innovative ideas in pH and conductivity measurement and easy use.
This is the First Perfect Combination.

XS
INSTRUMENTS



If you have a beautiful bench meter, but you don't combine it with a perfect pH electrode, this will be always and only a simple instrument that shows only numbers on the display and not pH measurement. Also in this case we have worked for a perfect combination. A very famous Swiss producer has developed, only for XS instruments, a complete laboratory line of pH electrodes for every type of application.
This is the Second Perfect Combination.

XS
INSTRUMENTS



"The calibration of the measuring system is one of the most important factors. To ensure a high measuring accuracy one has to follow the correct calibration procedure, use new and accurate buffer solutions and wait long enough for stable indication values of the electrode assembly to be calibrated. No measurement can be more accurate than its calibration accuracy" (International of basic and General Terms in Metrology)
If you have a good electrode, but you don't calibrate it with buffer solutions with good metrological traceability, You can't obtain reliable results. The XS buffer solutions come to celebrate the third Perfect Combination.
A Perfect Combination for new emotions.

pH, Conductivity, Oxy and ORP instruments

XS
INSTRUMENTS



GUARANTEED BY:

GIORGIO BORMAC
S.r.l.

COMPANY WITH SYSTEM
OF QUALITY MANAGEMENT
UNI EN ISO 9001: 2015
CERTIFIED BY CERTIQUALITY



DISTRIBUTED BY:

